


Molecular & Cellular Proteomics

Volume 7, Number 6, June 2008

www.mcponline.org

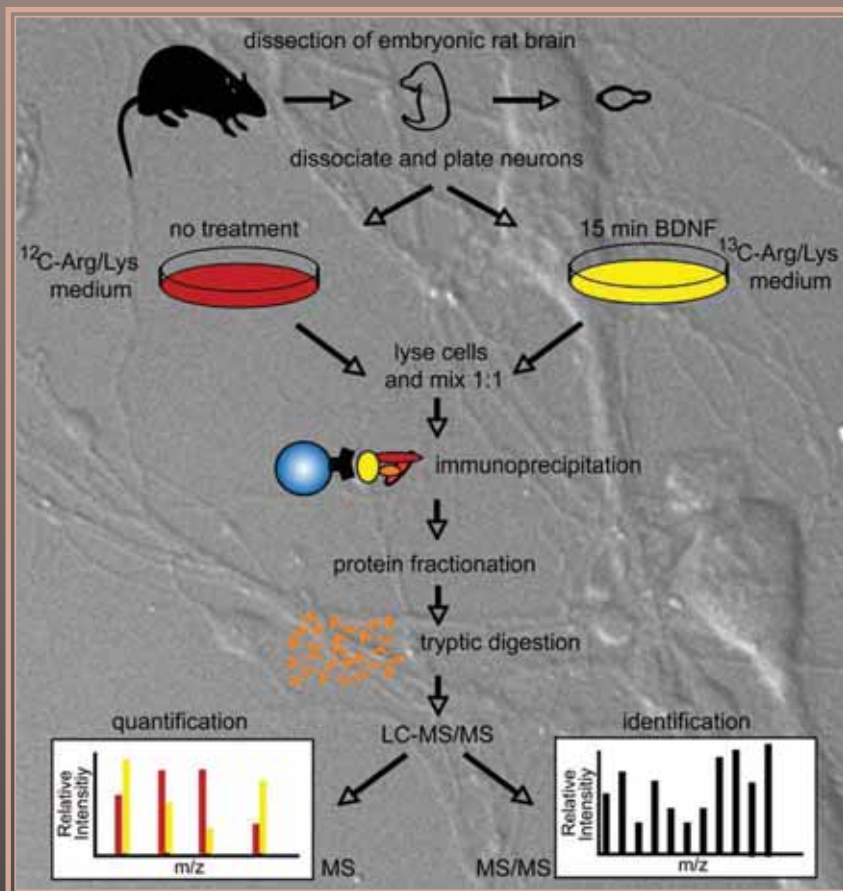

Stable isotope labeling by amino acids in primary neurons

In this issue

Atenolol Unraveled by LC-MS/MS
Aquaporin Phosphorylation
Novel Rab Effector Screening
Proteomics Data Confidence
Proteomics of Photoreceptors
SILAC in Primary Neurons
Kinase Inhibitor Evaluation
A Screen for DAPk Substrates
CFTR Pharmacology Interactions
Fasciola Cathepsin L Proteases
Accurate Peptide ID by PE-MMR
The Probability Ratio Method
Amphiphysin Phosphosites
Head-and-Neck Cancer Biomarkers
Colorectal Cancer Cells
CNHUPO: Pioneer Sino-Proteomics



Published by the American Society
for Biochemistry and Molecular Biology

Endorsed as an
Official Journal of
HUPO
Human Proteome Organisation

When Performance Matters



PICOTIPS®

Nanospray Emitters

Regardless of which method your analysis requires—online or offline—New Objective has the emitter to meet the high sensitivity demands of nanoESI.

New Objective emitters are precision-manufactured and machine-tested for shape, size and integrity. Only those emitters that meet our very tight specifications are then packaged in our unique, adhesive-free containers for delivery.

New Objective emitters are available with different conductive coating options to match your systems' voltage application method.

UPNS™ Ultra-Performance NanoSpray
Highest grade of performance, efficiency and flexibility in LC-MS analysis.

NO ADHESIVE PACKAGING

Revolutionary Patent-Pending design utilizes no adhesives and is extremely rugged and user-friendly. Each package ships with disposable tweezers for increased safety to user and emitters.

ONLINE NANOSPRAY

Online analysis is characterized by continuously pumped mobile phase at low flow rates through an emitter – most commonly provided via syringe pump or LC pump. High voltage is applied to the mobile phase to generate spray for sample delivery to the mass spectrometer.

OFFLINE NANOSPRAY

Offline analysis is characterized as loading a discrete sample, usually by syringe or pipette, into an emitter that is then mounted into the nanospray source. Sample flow is generated by electrostatic attraction of the liquid inside the emitter, which has been charged by high voltage.

